

# EU Quality Management System Certificate

Regulation (EU) 2017/745, Annex IX Chapter I and III

## MDR 801167 R000

**Manufacturer:** Well Lead Medical Co., Ltd.

**Address:**

C-4 Jinhu Industrial Estate  
Hualong Panyu  
Guangzhou  
Guangdong  
511434  
China

**Single Registration Number:** CN-MF-000006728

**EU Authorised Representative:** Shanghai International Holding Corp. GmbH (Europe)


**Address:**

Eiffestrasse 80  
Hamburg  
20537  
Germany

**Scope:** See attached **Device Schedule**

On the basis of our examination of the quality system in accordance with Regulation (EU) 2017/745, Annex IX Chapter I and III, the quality system meets the requirements of the Regulation. For the placing on the market of Class III devices, and Class IIb implantable devices that are not considered well-established technologies as specified in Article 52(4) an additional Annex IX Chapter II certificate is required.

For and on behalf of BSI, a Notified Body for the above Regulation (Notified Body Number 2797):



Graeme Tunbridge, Senior Vice President Medical Devices

First Issue Date: **2023-12-14**

Current Issue Date: **2023-12-14**

Starting Validity Date: **2023-12-14**

Expiry Date: **2028-12-13**

...making excellence a habit.™


# EU Quality Management System Certificate

Regulation (EU) 2017/745, Annex IX Chapter I and III

## MDR 801167 R000

### Device Schedule: Class III and Class IIb devices

| Class IIb                   | Intended purpose                                                                                                                                                                                                                          |
|-----------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Latex Foley Catheter        | Latex Foley is inserted into the bladder through urethra and are indicated for routine urine drainage or for routine post-operative drainage and irrigation bladder.                                                                      |
| All Silicone Foley Catheter | All Silicone Foley Catheter is intended to be used by trained person or trained medical staff for drainage and/or irrigation of the patient bladder by inserting the catheter into the vesical cavity of the bladder through the urethra. |

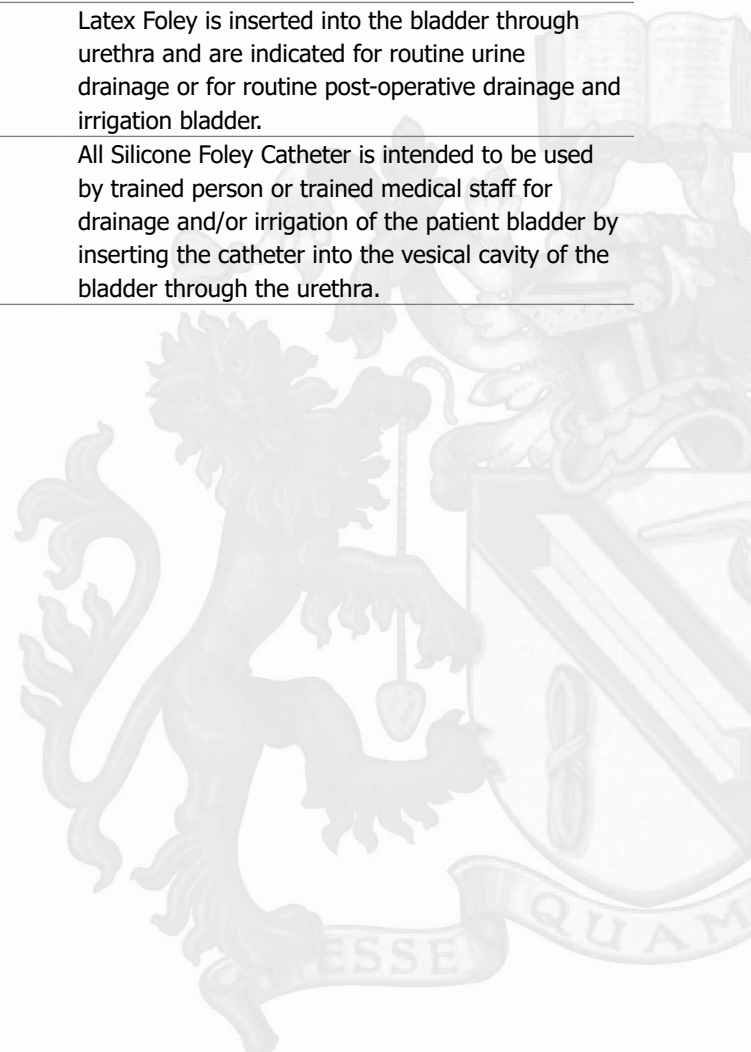

First Issue Date: **2023-12-14**

Current Issue Date: **2023-12-14**

Starting Validity Date: **2023-12-14**

Expiry Date: **2028-12-13**

...making excellence a habit.™

Page 2 of 3

Validity of this certificate is conditional on the Manufacturer's quality system being maintained to the requirements of the Regulation as demonstrated through the required surveillance activities of the Notified Body.  
This certificate was issued electronically and is bound by the conditions of the contract.

NB Contact: BSI Group The Netherlands B.V., Say Building, John M. Keynesplein 9, 1066 EP, Amsterdam, Netherlands. Tel: + 31 (0) 20 346 07 80  
Corporate Contact: BSI Group Assurance Limited, registered in England under number 05435540 at 389 Chiswick High Road, London, W4 4AL, UK.  
A Member of the BSI Group of Companies.

# EU Quality Management System Certificate

Regulation (EU) 2017/745, Annex IX Chapter I and III

**MDR 801167 R000**

## Certificate History

(References to applicable Common Specifications, Harmonized Standards complied with, and the relevant test and audit reports that support any of the below certificate changes may be requested from [Certificate.Verification@bsigroup.com](mailto:Certificate.Verification@bsigroup.com))

| Date    | Reference Number | Action |
|---------|------------------|--------|
| Current | 30056657         | Issued |



First Issue Date: **2023-12-14**

Current Issue Date: **2023-12-14**

Starting Validity Date: **2023-12-14**

Expiry Date: **2028-12-13**

...making excellence a habit.™

Page 3 of 3

Validity of this certificate is conditional on the Manufacturer's quality system being maintained to the requirements of the Regulation as demonstrated through the required surveillance activities of the Notified Body.

This certificate was issued electronically and is bound by the conditions of the contract.

NB Contact: BSI Group The Netherlands B.V., Say Building, John M. Keynesplein 9, 1066 EP, Amsterdam, Netherlands. Tel: + 31 (0) 20 346 07 80  
Corporate Contact: BSI Group Assurance Limited, registered in England under number 05435540 at 389 Chiswick High Road, London, W4 4AL, UK.  
A Member of the BSI Group of Companies.